







Vestfrost Solutions is working towards reaching the UN - Global Sustainable Development Goals by 2030.

The Sustainable Development Goals are the blueprint to achieve a better and more sustainable future for all.

In order to implement Goal no 12 "Responsible Consumption and Production", this manual has been printed on recycled paper.

Technical manual VLS174A AC



WARNING

As the appliance contains flammable refrigerant, as stated on nameplate, it is essential to ensure that the refrigerant pipes are not damaged.

The quantity and type of the refrigerant used in your appliance is indicated on the rating plate.

Standard EN378 specifies that the room in which you install your appliance must have a volume of 1m³ per 8 g of hydrocarbon refrigerant used in the appliances. This is to avoid the formation of flammable gas/air mixtures in the room where the appliance is located in the event of a leak in the refrigerant circuit.

WARNING:

Keep ventilation openings in the appliance or in built-in structures must be kept clear.

WARNING:

Do not use other mechanical devices or means to accelerate the defrosting process or to remove rime other than those recommended by the manufacturer.

WARNING:

Do not damage the refrigerant system.

WARNING:

Do not use **electrical appliances** inside the refrigerated storage compartment, unless they are of a type recommended by the manufacturer

WARNING:

Do not expose the appliance to rain, and secure not splashing water when cleaning the floor.

WARNING:

This appliance is not intended for use by persons (including children) with reduced physical, sensory or mental capabilities, or lack experience and knowledge, unless they have been given supervision or instructions concerning use of the appliance by a person responsible for their safety. Children should be supervised to ensure that they do not play with the appliance.

WARNING:

Children must not play with, on, or around the appliance.



WARNING:

Children must not clean the appliance or carry out general maintenance unless they are at least 8 years old and are being supervised.

WARNING:

Danger risk of fire or explosion. Flammable refrigerant used, as stated on nameplate. To be repaired only by trained personnel



WARNING:

Do not store explosive substances such as aerosol cans with a flammable propellant in this appliance.

WARNING:

Sharp edges on cabinet, compressor compartment, evaporator, ventilation cover and on internal equipment can occur. Please be aware to avoid injury.

WARNING:

The condenser on the back of the appliance will in some cases have a hot surface. Please be aware to avoid injury.

WARNING:

Appliance use flammable insulation blowing gas. For information about safe disposal, please contact your local disposal service. See section for Disposal.

GB

Contents

WARNING	2
Periodic preventive maintenance checks	5
Complete spare part list VLS174A AC	6
Vital components	8
Health and safety guidance - Warning!	9
Required basic tools	.10
Wire diagram - VLS 174A AC	11
Voltage stabilizers	.12
Safety instructions - Installation	.15
Installation and maintenance work	.16
Fuse trouble shooting	.17
Maintenance, diagnostic and repair procedures	.17
Motor compartment	.18
Thermostat replacement	.19
Thermostat adjustment	.23
Circuit breaker replacement	.24
Thermostat sensor replacement	.25
Sensor replacement for Icebank	.27
Connection of heating element	.28
Starting device replacement	.29
Run capasitor replacement	.31
Thermometer replacement	.32
Voltage Stabilizer ECU replacement	.35
Transformer replacement	.36
Compressor replacement	.37
On-site checklist	.38
Trouble shooting	.39
Technical support	.40
Recycling procedures	.41

Periodic preventive maintenance checks

Daily Check:

Monitor Temperature Internal lid is placed properly Lid fits and lock tight to cabinet Lid gasket not faulty.

Weekly maintenance:

Remove any water at the bottom of the refrigerator with a cloth. Wipe of water droplets on the inside wall.

Monthly maintenance:

Clean grille for compressor compartment. Clean the refrigerator with lukewarm water and mild detergent.

Yearly maintenance:

Check electrical connections and components.


PQS Code	Model	PQS Performance specifications Specification reference:	PQS Independent type-testing protocol Product verification protocol:
E003/120	VLS174A AC	E003/RF03.4	E003/RF03-VP.3

5




Complete spare part list VLS174A AC

Position	Item number	Item name
0061	0-6538001	Filter drier,
0087	0-6038175	Base plate fittings, complete
0129	8-036510018	Compressor - HXK80AT , Complete,
0153	7535234	Mains lead/Power cord UK plug with angled C13 connector
0153	7535250	Power cord
0153	7535254	Power cord EU H05VV-F 3G1 C13 jack 90° black 2500mm EU-
0550	6520510	Run cap. 4uF/4,8 receptacles
1126	0-A921012	Cover + wirring clamp
2170	0-A9301260103	Distance piece
2431	A915010	Lock complete snap locks
5000	3010049	Drain plug
5013	3040400	Adjustable foot
5052	2042052-01	Mounting plate for condenser VLS024
5057	6010436	WOT condenser
5144	520002400170	Lid
5402	1510059	Hinge
5450	3011135-01	Top part for hinge cover
5451	3010032-01	Bottom part for hinge cover
5578	2043682-01	Motor screen
5582	3510517	Basket VLS048/HFK048
5583	3510518	Bottom grating VLS048/HFK048
5606	8090054	Inlay for handle,
5606	8090342-94	Inlay for handle,
5682	1510255	Nikel-plated Key
5705	7020406	Temperature monitoring device Fridge-Tag 2E
5709	7060104	Frame for cover rocker switch bezel
5712	702090041	Safety, Thermostat XR01CH incl. sensor
5712	702090054	Refrigerator, Thermostat XR30CH incl. sensor
5714	7060247	Overcurrent circuit breaker
5718	7060105	Rocker Switch Cover
5730	7020245	"on-off" switch
5738	7010138	Pilot lamp, green
5756	7020382-03	Thermometer, solar
5883	7020475	Voltage stabiliser controller thyratron MFSL 110-285V 50Hz
5884	7020497	Voltage stabilizer transformer thyratron MFSL 110-285V 50Hz
6550	7080143	Connector



GB

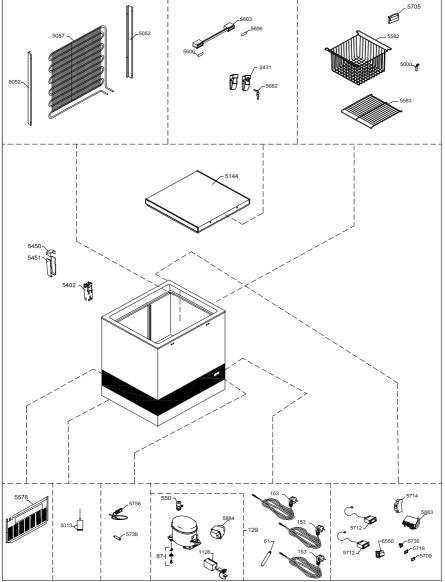



Vital components

Positior	n Item no	Description	
0129	8-036510018	Compressor	
5712	702090041	Safety,Thermostat XR01CH incl. sensor	
5712	702090054	Refrigerator,Thermostat XR30CH incl. sensor	
0550	6520510	Run capacitor	
1126	0-A921012	Cover og wire clamp	
5883 5884	7020475 7020497	Controller Thyratron Transformer Thyratron	

Health and safety guidance – Warning!

Before any repair job be aware of following!

WARNING:

Before servicing or cleaning the appliance, disconnect it from power source.



WARNING:

Danger risk of fire or explosion. Flammable refrigerant used. To be repaired only by trained personnel.



Required basic tools

1.Flexible socket wrench - size 7+13mm

2.Nose plier

3.Screwdriver - size 1,0x6,0 + 0,6x3,5

4. Phillips screwdriver

5.Torx screwdriver - size T10 + T20

6.Clamp meter


7.Multimeter

Proposed additional service kit/items Sealing kit Tar tape Extra self-tapping screws



GB

Wire diagram - VLS 174A AC

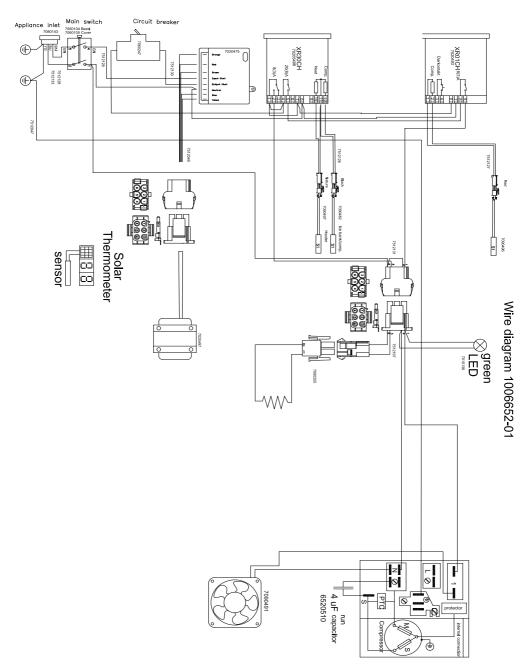



Voltage stabilizers


Getting to know your appliance


Product features:

- Voltage stabilizer
- Voltage, Frequency and current supervisor
- Intelligent ambient temperature protection
- Intelligent Time delay 3'30"+0"to30" random
- Surge protection
- Reconnecting Voltage Hysteresis
- Zero Crossing
- Soft Start
- Zero current change over

Electronic Control Unit - ECU & Trafo

(1): "OUT OF LIMITS" led (Red) (3), (6): Mounting points (2): "OPERATION" led (Green) (4): Fast on terminals (5):Connection cables - Fast On female terminal









LED - Indication

Event	Red LED	Green LED
Normal operation	Off	On
4 minutes delay	Blink slow	Off
Frequency out of limits	Blink fast	Off
Temperature out of limits	Blink slow	Blink slow
PPS MFS Failure or No Power	Off	Off

Voltage stabilizasion

Output Vo	oltage Limits
PPS MFS-L performs voltage correction and stabilization using Autotransformer, Relays and Triacs. PPS MFS-L makes switching in order to keep the output voltage within limits.	200 - 245 VAC ±2%

Voltage & frequency monitoring

Input Voltage lir	nits
PPS MFS-L monitors voltage and frequency of main po- wer and cuts off the output when the values of main power (voltage or frequency) come out of limits.	60 - 415 VAC

	Input frequency limits				
Stage \ Hz	50 Hz	60 Hz			
Stage_1: Continuously Operation	47 - 53	57 - 63			
Stage_2: 60mins Delay to Cut-Off	46 - 47 & 53 - 54	56 - 57 & 63 - 64			
Stage_3: 10mins Delay to Cut-Off	45 - 46 & 54 - 55	55 - 56 & 64 - 65			
Stage_4: Instant Cut-Of	< 45 & > 55	< 55 & > 65			

	PPS MFS-Lw Series :					PPS MFS-1Lw			IM Sdd	PPS MFS-2Lw
PPS MFS-xxxLi	PPS MFS-xxxLw Series (xxx: 070, 085, 100, 150, 200)	00)		040	090	020	085	100	150	220
ú	Nominal Voltage						220 - 240 VAC			
Sunnly	Operation Voltage Bandwidth (@ $25^{0}C$)	th (@ 25 ⁰ C)					60 - 415 VAC			
hindho	Ambient Temperature	Hun	Humidity		-5 to +45 °C	°C		5 - 95 %RH	5 - 95 %RH, non-condensin	'n
+	Voltage	Low	High	11(110 VAC ± 3% with hysteresis	h hysteresis		285 VAC ±2	285 VAC ±2% with hysteresis	sis
Input	Frequency Lower / Upper	50Hz	ZH09		45 / 55 Hz ±0.2Hz	:0.2Hz		55 / 6	55 / 65 Hz ±0.2Hz	
	Voltage range					2(200 - 245 VAC ±2%	2%		
Outnut	Max. Current (A)							4.3		
2	Continuous Operation (45°C) Current (A) @ Low Voltage) Current (A	.) @ Low					3.2		
Start Up Time, Time Delay	Time Delay			 4 minutes 2ero on Pi 	 4 minutes (3'30'' + 0" to 30'' random) Zero on Production Line for first 30 mi 	0 30'' random) for first 30 mii	iutes continuo	 4 minutes (3'30" + 0" to 30" random) 2ero on Production Line for first 30 minutes continuous operation of life cycle 	life cycle	
Thermal protection	ction			 Temperat Temperat 	 Temperature limits +80 °C Temperature rise 15°C / 15 minutes 	°C 15 minutes				
Plastic Housing	50					UL94	UL94 V-0 Flame Retardant	ardant		
IP Class							IP44			
Lifetime						Relay l	Relay lifetime cycles 350,000	350,000		
Connections						6.3mm	6.3mm x 0.8mm flat, terminal	terminal		
Cable Harness - Lengths	- Lengths					250mm / 5	250mm / 550mm / 1000mm versions	mm versions		
Insulation Clas	Insulation Class, Transformer Windings						H (180°C)			
		ECU					114 x 98 x 31			
Dimension (mm)	n) Trafo	Standard Vertical i	Standard installation Vertical installation					130x95x110 108x140x90		
Total weight (Kg)	(g)							4.3		

Specifications

GB

Safety instructions - Installation

What this chapter contains

This chapter contains the safety instructions which you must follow when installing, operating and servicing the Power Protector Stabilizer MFS. If ignored, physical injury or death may follow and/or damage may occur to the PPS MFS. Read the safety instructions before you work on the unit. These warnings are intended for all who work on the PPSMFS, or cable,



WARNING! The work described in this chapter may only be carried out by a qualified electrician.lgnoring the safety instructions can

cause physical injury, death or/and damage to the equipment. Make sure that the device is disconnected from the mains (input power) during installation.

Beware of hot surfaces. Some <u>/ss</u>/ parts, such as transformer, may remain hot for a while after disconnection of the electrical supply.

- Only qualified personnel are allowed to install and maintain the PPS MFS.
- PPS MFS is intended to be built into commercial refrigeration appliances or other enclosures that provide protection against certain external influences and, in any direction, protection against direct contact and electric shock.
- It shall be installed in an area where it is inaccessible without disassembly of the enclosing area.
- Never work on the PPS MFS or cable when main power is applied. Always ensure by measuring with a multimeter (impedance at least 1 Mohm) that voltage between device input phases INPUT and NEUTRAL is close to 0V. Externally supplied control circuits may cause dangerous voltages inside the device even when the main power on the drive is switched off.
- Do not make any insulation or voltage withstand tests on the device.
- When reconnecting the wiring, always check that the Phase - Neutral order is correct.
- Do not change the electrical installations of the PPS MFS. Changes may affect the safety performance or operation of the device unexpectedly. All customermade changes are on the customer's responsibility.
- Make sure that dust from borings and grindings does not enter the drive when installing. Electrically conductive dust inside the unit may cause damage or malfunctioning.
- Do not fasten the device by welding. Note: The fast-on terminals on the device are at a dangerously high voltage when the input power is on.



Installation and maintenance work


- The PPS MFS consist of two parts, the Electronic Control Unit (ECU) and the Autotransformer (Trafo). The ECU and the Trafo of the device is delivered in separates cardboard box. The type, size and material of the package depend on the frame size of the Autotransformer.
- The parts of the PPS MFS must be connected by using fast-on terminals taking in care the coloring code of the cables and ECU.
- PPS MFS is intended to be used with the protection of a fuse gG, type B, IEC60269-3-1.
- Confirm compatibility with connection terminals as well as insulation. The connectors are Fast On terminals 6.3x0.8mm
- The device must be installed in an upright position (beside figure) with allowance for adequate cooling.

IP rating is met only when the ECU is installed in a vertical position with the connection tabs at the bottom. This is also important as the ECU also detects ambient temperature as one of its features.



• An earth ground connection must be take place on to the Trafo. Detail of grounding Transformer Enclosure during implementation in the appliance.

(IEC 60417-5019)



Before powering the device:

- Confirm color coding between ECU and Autotransformer
- Confirm the correct fitting of the terminals to ensure IP rating of the connections.



Fuse trouble shooting

How to determine why the thermal magnetic breaker nuisance trips?

The thermal magnetic breaker is installed to protect the build-in voltage stabilizer.

Cause: Circuit breakers trip.

Resolution:

- 1. First, determine if the breaker trips on startup or if it trips after running for a while.
- If it trips at start-up but doesn't do it repeatable, it is caused by inrush current to either the voltage stabilizer or the compressor. Resetting the breaker will have no harm on the appliance
- 3. If it trips at start-up and does it multiple times, there is a short circuit within the appliance and a service technician should be contacted.
- 4. If it breaks after some time, the appliance is overloaded. Ensure that the condenser and engine room are clean and give the unit some minutes to cool down before resetting the fuse. The start electronic on the compressor can also be faulty causing the compressor to run on the start condenser constantly.

Maintenance, diagnostic and repair procedures

The PPS MFS maintenance-free and is made up of non-repairable / refurbishable parts. In the event of a failure of the PPS MFS, both ECU and Trafo have to be replaced with new unused units. Part replacement is not advisable.

Storage

Should not be stored or and transport in high temperature or high humidity condition. Usage, beyond the specified shelf life could compromise product long term reliability. The suitable condition is +5 to +35°C and less than 95% RH in Relative Humidity indoor.

Applicable Ambient temperature and humidity range during transport and storage: -30 to +70°C, 5 to 95% RH.

End of life resource recovery and recycling procedures.

Disposal of Old Electrical & Electronic Equipment (Applicable in the European Union and other European countries with separate collection systems).

> This symbol on the product or on its packaging indicates that this product shall not be treated

as household waste. Instead it shall be handed over to the applicable collection point for the recycling of electrical and electronic equipment. By ensuring this product is disposed of correctly, you will help prevent potential negative consequences for the environment and human health, which could otherwise be caused by inappropriate waste handling of this product.



GI

1.Use a screwdriver to loosen the 4 screws.








2.Gently pull the compressor grille.



Thermostat replacement

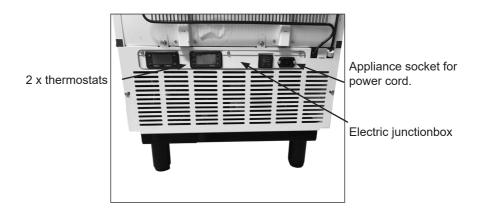




Front with display and adjustments buttons for safety



Front with display and adjustments buttons for cooler



Back with electrical sockets



Top view





1. Access electrical components Dismount 3 x Torx 20 screws and unmount the junc-




2. Pull out the box gently


tion box lid




3. Loosen the 3 x 20 screws on the side were the circuit breaker is place



4. Remove grounding cable from junction box by unscrewing bolt with a wrench 6mm




5. Remove 2 fixing clamps from thermostat. Slide the fixing clamps backwards



Fixing clamp






6. Use your finger to press and slide the lower clamp backward to remove form the thermosatat body




8. Switch the sensor wire plug from old socket to the new thermostat socket.




7. Push the thermostat out



9. Switch the power wire plug from the old to the new thermostat wire socket.



10. Bring the thermostat back in place.




11. Use your finger to press and slide the upper clamp back in place to secure fixture of the thermostat.



12. Remount grounding wire.



13. Remount junction box cover.



It's the same procedure that needs to be done for both of the thermostats





Safety thermostat Cooler thermostat



SET To display target set point in programming mode it selects a parmeter or confirm an operation.

(DEF) To start a manual defrost (UP) To see the max. stored temperature, in programming mode in browses the parameter codes or increases the displayed value.

✓ (DOWN) To see the min. stored temperature, in programming mode in browses the parameter codes or decreases the displayed value.

 $^{(1)}$ To swich the instrument off, if onF=oFF.

Not enabled.

 $\stackrel{\curvearrowleft}{\to} + \stackrel{\bigtriangledown}{\bigtriangledown} \text{ To lock & unlock the keyboard.}$

Deafault Set Points

Safety thermostat
Cooler thermostat

SP = 2,5 SP1= 5 /SP2= -5

IMPORTENT:

Incorrect parameter settings can lead to unsatisfactory cooling, risking damage to stored vaccines. If adjustment is required ONLY to be performed by trained technicians.

Adjust the controller max. 1°C at a time. After adjustment monitor appliance carefully for min. 24 hours.

Main functions

How to see the setpoint

- 1. Push and immediately release the SET key the display vill show the Set point value.
- Push and immediately release the SET key or wait for 5 seconds to display the probe value again.

How to changes the setpoint


- 1. Push the SET key for more than 2 seconds to changes the Set point value
- The value of the set point will be displayed and the °C or °F LED starts blinking
- 3. To change the Set value push the o or n arrows within 10s
- 4. To memorise the new set point value push the SET key again or wait 10s.




Circuit breaker replacement




Circuit breaker is placed on the back side of the dixell. Pull out the box gently




2. Used Torx 20 to loosen the screw




1. Dismount 6 x Torx 20 screws and unmount the junction box lid



3. Remove the fitting



4. Remove the wires



3. Pull the circuit breaker out and replace it.


Thermostat sensor replacement




The thermometer sensor is placed inside the compartment of the appliance.



2. Sensor probe / Grab the wire and pull it out gently




4. Gently pull the white wire until the probe is visible.



1: Dismount the temperature sensor cover by loosen the 2 x torx screws – size 10.




3. In Compressor compartment, remove black sealing, and gently pull the white wire until the probe is visible.



5. The thermostat sensor comes with probe, wire and cable socket.




 IMPORTANT! When re-mounting the new thermostat sensor remember to properly seal the wire feed through.



7. **IMPORTANT!** When re-mounting the new thermometer make sure the wire is placed properly.


Sensor explanation

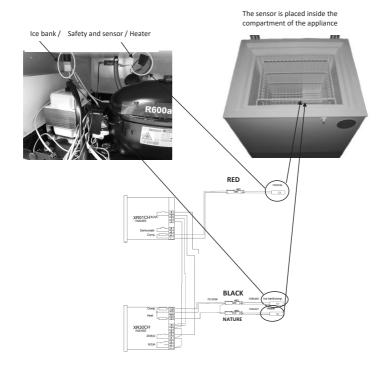

Sensor replacement for Icebank




The icebank sensor is placed in the corner



Mark on wire

End cap on wire




1. Put the wire into the pipe with the cap end.Pull it into where the mark on the wire



2. Tie it up with strips and cover with tar kit



Starting device replacement



Front with terminals.



Side view.



Back with connection plug.



The starting device is mounted on the left side of the compressor.



1. Dismount the cover by pushing the cover lock from right to the left with a flat screw driver.



2. Pull out the cover to remove


GB




3. Use a screw driver to losen 3 x screws.



4. Use a screwdriver to loose the starting device from socket and pull.




- 5. Use a nose plier to unmount the wire sockets from starting device.
- 6. Exchange the wires 1/1 from the old starting device to the new one.

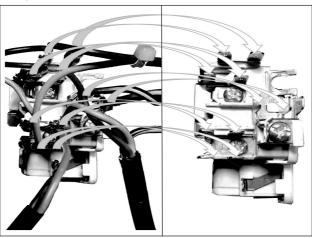



Run capasitor replacement



The run capasitor is placed in the left side of the compressor compartment, fixed to the compressor bracket.




2. Pull out the cover to remove



1. Dismount the cover by pushing the cover lock from right to the left with a flat screw driver.



3. Flip out the clamp to free the capasitor from the bracket.



4. Use a nose plier to unmount the wire sockets.



5. Loosen the screw for cord relieve and pulle out the wire. The capasitor kan be remounted in reverse ordrer.

Thermometer replacement



The thermometer is placed in at the front of the appliance.




The thermometer sensor is placed inside the compartment of the appliance.



2. Sensor probe / Grab the wire and pull it out gently




Thermometer display.



1: Dismount the temperature sensor cover by loosen the 2 x torx screws – size 10.



3. In Compressor compartment, remove black sealing, and gently pull the white wire until the probe is visible.



4. Gently pull the white wire until the probe is visible.



5. Use a screw driver to gently push the socket of the thermometer.



6. Temperature monitor is loose from cabinet.



7. Thermometer comes with wire and sensor.



8. Installation of thermometer display.



9. Push untill display is fixed to cabinet.





10. Thermometer display is in place.




11. **IMPORTANT!** When re-mounting the new thermometer remember to properly seal the wire feed through.



 IMPORTANT! When re-mounting the new thermometer make sure the wire sealing plug is placed properly.




Voltage Stabilizer ECU replacement



1. The controller is placed in the bottom



2.Loosen the 2 screws and remove the wires



3.Used a flexible socket wrench




4. Exchange the wires from the old ECU to the new.




Transformer replacement




1. The transformer is placed on the left sideof the compressor compartment



3. Used a torx T20



2. Loosen the screw



4.Part the transformer power wires, bysqueezing on the side of the clamps fixingthe wire connection, the pull the plug/socketapartthe



5. Pull out the voltage stabilizer tranformer



Compressor replacement

Procedure of compressor switch.

- 1: WARNING! Drain coolant R600a from refrigeration system by vacuum suction.
- 2: **IMPORTANT!** Blow refrigeration system with NO/Nitrogen
- 3: Cut
 - A: Suction and pressure tube
 - B: Capillary tube
 - C: Dry filter
- 4: Dismount starting device
- 5: Dismount old compressor
- 6: Insert new compressor
- 7: Solder
 - A. Suction and pressure tube
 - B. Capillary tube
 - C. Dry filter
- 8: Install starting device

IMPORTANT! When solder copper tubes to iron tubes use silver tin

Filling of new refrigerant

- 9: Drain refrigeration system by vacuum suction
- 10: Check type sticker for required amount of R600a to fill on refrigerant system

On-site checklist

- Is the green diode in the control panel on (Power check)
- Temperature records (manual records, FT2 data)
- Is the internal temperature inside the acceptable range of +2° to +8°
- Is the vaccine compartment clean and without condensation (water)
- Is the Compressor running
- · Is baskets used and in place
- Is the appliance placed according to instruction in the manual.
- Does the lid close tight to cabinet and is the lid gasket in good condition
- Is the grille for compressor compartment clean
- Is all electrical components working properly
- Over all condition of the cabinet –internal and external: any corrosion, rusting, cracks
- Condition of the cables from the panel to the compressor including the lightening protection
- Inspection of the refrigeration line (the condenser, evaporator, the whole refrigeration circuit/line)




Trouble shooting

Fault	Possible cause	Remedy
Compressor is not running.	Be patient, it is most likely that the compressor will start within a	If this is not the case, check the following:
	few minutes.	- Check that power is connected and that the wire from the solar panel to the appliance is intact.
		- If the above is OK, call techni- cal supervisor.
Compressor is run- ning, and the tempe- rature is too high.	The ventilation grille is blocked.	Ensure unhindered air circula- tion.
	The lid is not closed properly.	Ensure that the lid is closed properly.
	The temperature in the room in which the appliance is installed is too high.	Shield the appliance against direct sun light and ensure more ventilation to the room.
No temperature is displayed.	The Thermometer is broken.	Change the thermometer.
	There is not enough light for the solar sensor.	Turn on the light.

Technical support

When contacting Vestfrost Solutions technical support please supply below information:

- 1. Model
- 2. Serial number
- 3. What is the issue

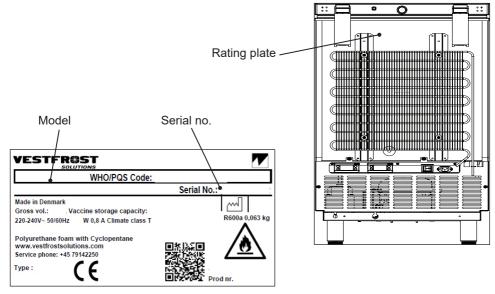

Contact:

Vestfrost Solutions

Tel. +45 75142250

cce-service@vestfrostsolutions.com

Or visit our service-center webpage:

http://www.vestfrostsolutions.com/service-center/



Recycling procedures

Information for Users on Collection and Disposal Old Equipment and used Batteries



This symbol on the products, packaging, and/or accompanying documents mean that used electrical and electronic products and batteries should not be mixed with general household waste. For proper treatment, recovery and recycling of old products and used batteries, please take them to applicable collection points, in accordance with your national legislation and the Directives 2012/19/EU and 2006/66/EC.

By disposing of these products and batteries correctly, you will help to save valuable resources and prevent any potential negative effects on human health and the environment which could otherwise arise from inappropriate waste handling.

For more information about collection and recycling of old products and batteries, please contact your local municipality, your waste disposal service or the point of sale where you purchased the items.

Penalties may be applicable for incorrect disposal of this waste, in accordance with national legislation.